

**UAB**  
THE UNIVERSITY OF  
ALABAMA AT BIRMINGHAM  
Knowledge that will change your world

# Choosing the metabolomics platform

Stephen Barnes, PhD  
Department of Pharmacology & Toxicology  
University of Alabama at Birmingham  
[sbarnes@uab.edu](mailto:sbarnes@uab.edu)

**T**argeted  
**M**etabolomics &  
**P**roteomics  
**L**aboratory

1

## Synopsis


- **The analytical challenge**
- **Early days of metabolomics**
- **Platforms**
  - TLC
  - GC; GC x GC
  - GC-MS
  - LC-MS
- **Mass analyzers**
- **What is mass?**
- **The LC**
  - Selected ion monitoring
  - Multiple Reaction Ion Monitoring
- **Ion mobility**
- **Imaging-MS**

2

## Challenges

- Unlike DNA, RNA and proteins, the metabolome is phenomenally chemically diverse
- Ranges from a gas ( $H_2$ ) that prevades the universe and is the principal component of the Sun

to



- Earwax (long chain fatty acids, both saturated and unsaturated, alcohols, squalene, and cholesterol)
- No single method of analysis


3

## Early beginnings of metabolomics in London

- Sir Ernst Chain (1945 Nobel Laureate – the biochemist who characterized penicillin)
  - Also renown for his work on microanalysis
- Used 2D-paper chromatography to resolve glycolytic, Krebs cycle and amino acids derived from  $^{14}C$ -glucose
  - Geiger counter mounted on a typewriter frame
  - Digitized the collected data and prepared computer-generated figures




Keith Mansford

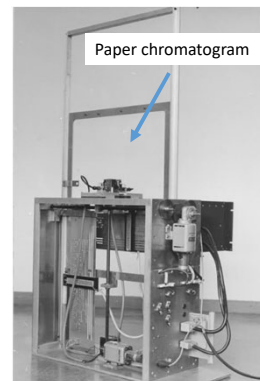


**METABOLOMICS**

4

## Radiochromatography examples

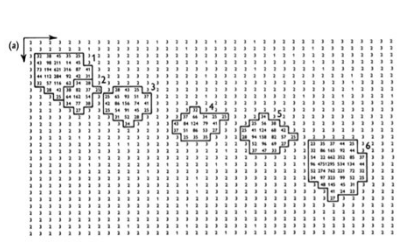

**J Physiol (1960) 154:39**  
**E.B. Chain, K.R.L. Mansford and F. Pocchiari**

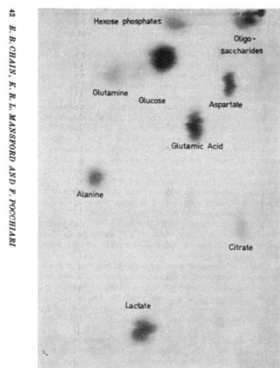


**Autoradiogram of <sup>14</sup>C-glucose metabolites from an isolated perfused Langendorff rat heart preparation. The metabolites were separated by 2D-paper chromatography.**

**The conditions were:**  
**1<sup>st</sup> dimension:** butan-1-ol-acetic acid-water (40:11:25, by vol.) for 16hr;  
**2<sup>nd</sup> dimension:** (-) phenol-aq. NH<sub>3</sub> (sp.gr. 0.88)-water (80:1:20, by vol.) for 24hr.

**Biochem. J. (1969) 115, 537**  
**E.B. Chain, K.R.L. Mansford and L.H. Opie**

5

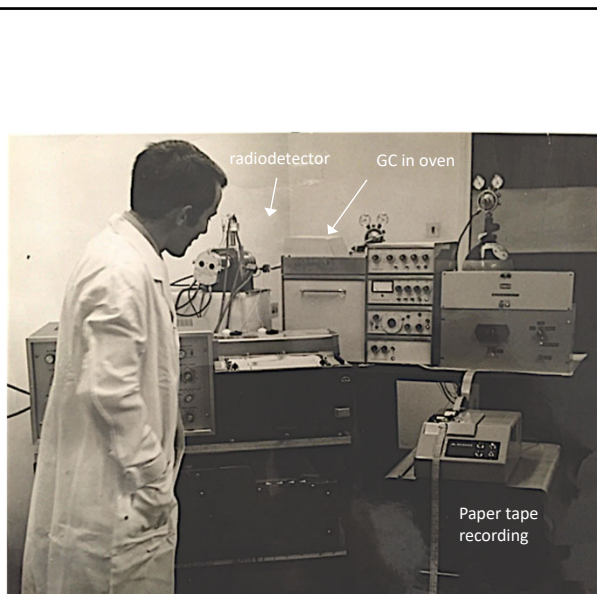

## Radio-GC analysis


metabolomics in its infancy

Radio gas-liquid chromatography with digitization of collected data


Developed this for my PhD work (1967-1970) to study glucose metabolism in acellular slime mold, *Physarum polycephalum*

6

## Radio-GC of Krebs cycle intermediates

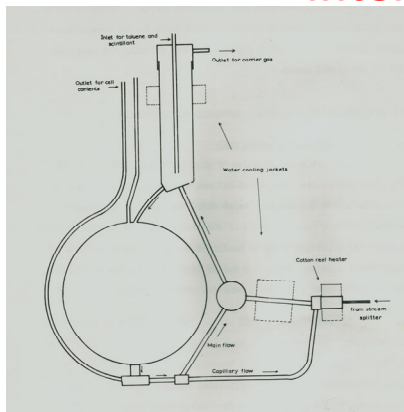

Popjak scintillation cell

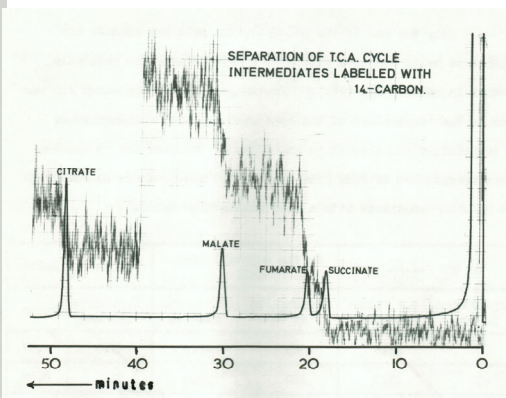

Stephen Barnes, PhD thesis


7

## Software for data analysis on a PDP9 computer

```


. DIMENSION Ibuff(1000), IDATA(725,2)
. COMMON Ibuff, IDATA, TIME, INT, SIG
. 5      ITIME=0
. 7      CALL TAPE(SIG, INTA)
. 8      IWRITE(1,1001)INTA
.      INT=INTA/300
. 10     NPOINT=1
. 11     CALL TAPE(SIG, IDATA(NPOINT,1))
.      IF (SIG.EQ.1) GO TO 16
.      IF (SIG.EQ.2) GO TO 13
.      WRITE(1,1001)NPOINT
. GO TO 11
. 13     IF (IDATA[1,1].GT.940) GO TO 11
.      IF (IDATA(NPOINT,1).EQ.0) GO TO 11
.      IF (NPOINT.EQ.725) GO TO 16
. 15     NPOINT=NPOINT+1
.      GO TO 11

```

Punched tape data  
1 data point/secDigital PDP computer  
Had a screen

8


## 2D-Thin layer chromatography of lipids KO of cerebroside sulfatase in kidney

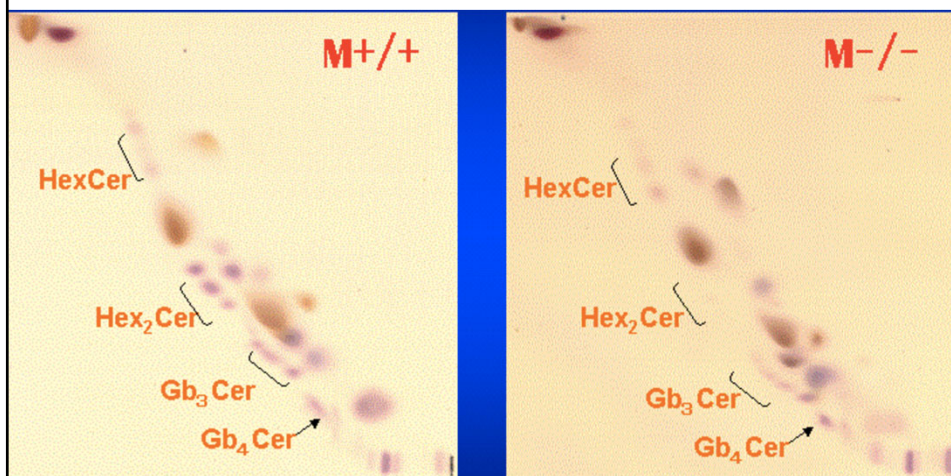

These days, TLC plates can be studied by direct electrospray ionization (DESI)

9

## Decision tree

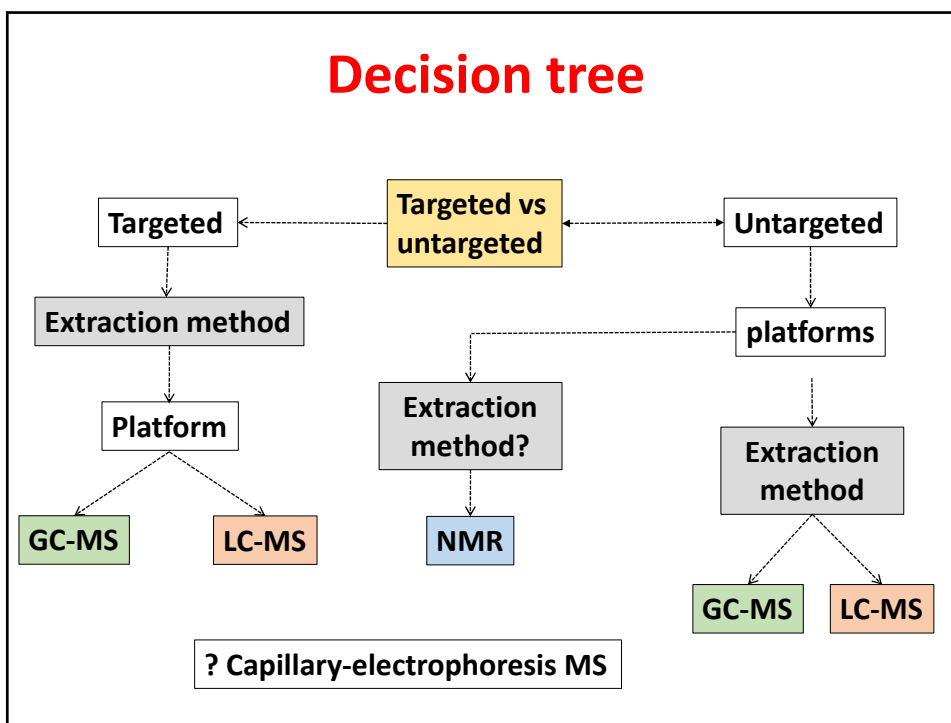


10

## Metabolomics and GC-MS

- **PROS**
  - Capillary columns can achieve very high chromatographic resolution
  - Retention times are reproducible
  - Mass spectral libraries are well developed
- **CONS**
  - Not all compounds can be analyzed by GC-MS
  - Although amino acids, sugars, fatty acids, amines and organic acids **can be derivatized**, complex polyphenol glycosides and polar lipids are too unstable, even when derivatized, at the temperatures used to elute them
  - Approximate mass limit of 400 Da

11




## Two dimensional GC to resolve metabolites

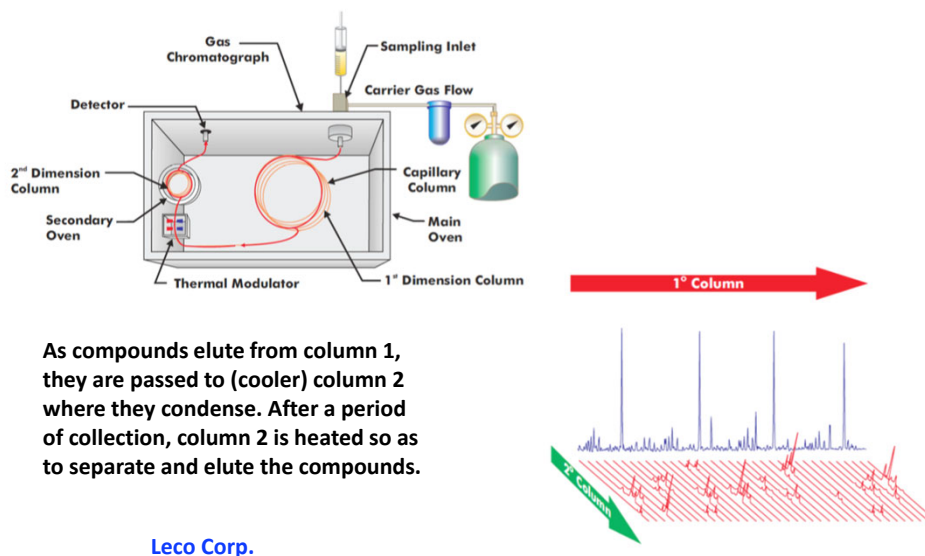

12

## Nuclear Magnetic Resonance (NMR) Spectroscopy

- Detects NMR active nuclei
- Robust and highly reproducible
- Non-destructive
- Quantitative
- Used in
  - Structure elucidation
    - Small molecules
    - Macromolecules (DNA, RNA, Proteins)
  - A number of techniques
    - 1D, 2D, 3D
  - Molecular motion and dynamics
- Similar method used in medical Imaging (MRI, fMRI)



from Wimal Pathmasiri

13

## NMR considerations

- **Sample amount:**
  - Typical 600 MHz instrument requires 0.5 ml plasma/serum
  - Higher field instrument and micro coil detector allows use of 0.1 ml
- **Quality control:**
  - In the UK Phenome Center, all samples are analyzed by NMR
    - This allows for detection of outliers
    - Also found that there is a correlation between the NMR spectrum and whether problems occur in LC-MS analysis
    - NMR analysis used to filter out these samples

14

## Hyperpolarization NMR

- **The NMR signal comes from the not-quite, non-equilibrium between the two or more energy states a nuclei experience in a strong magnetic field**
  - The natural excess population of the higher energy states is no more than 0.01%
  - This accounts for the low sensitivity of NMR
- **By hyperpolarizing the compound, the excess population can be increased by  $10^4$ - $10^5$ .**
  - Much increased sensitivity
- **Carbonaceous materials (metabolites) can be hyperpolarized by cooling to 1°K in a strong magnetic field (3 T or larger)**
  - However, the lifetime of the hyperpolarized state is quite short (10-30 s) making metabolomics experiments quite difficult

15


## Liquid chromatography-Mass Spectrometry

- **PROS**
  - **Almost all compounds can be analyzed by LC-MS**
    - Exceptions - hydrocarbons do not ionize
  - **Several orders of magnitude increased sensitivity compared to NMR**
  - **Can collect MS, MSMS and ion mobility data**
- **CONS**
  - **Not uniformly quantitative**
  - **Mass spectral libraries are not well enough developed**
  - **Chromatographic separation not adequate**
  - **Retention time reproducibility not as good as GC-MS**

16




## Mass spectrum of a compound

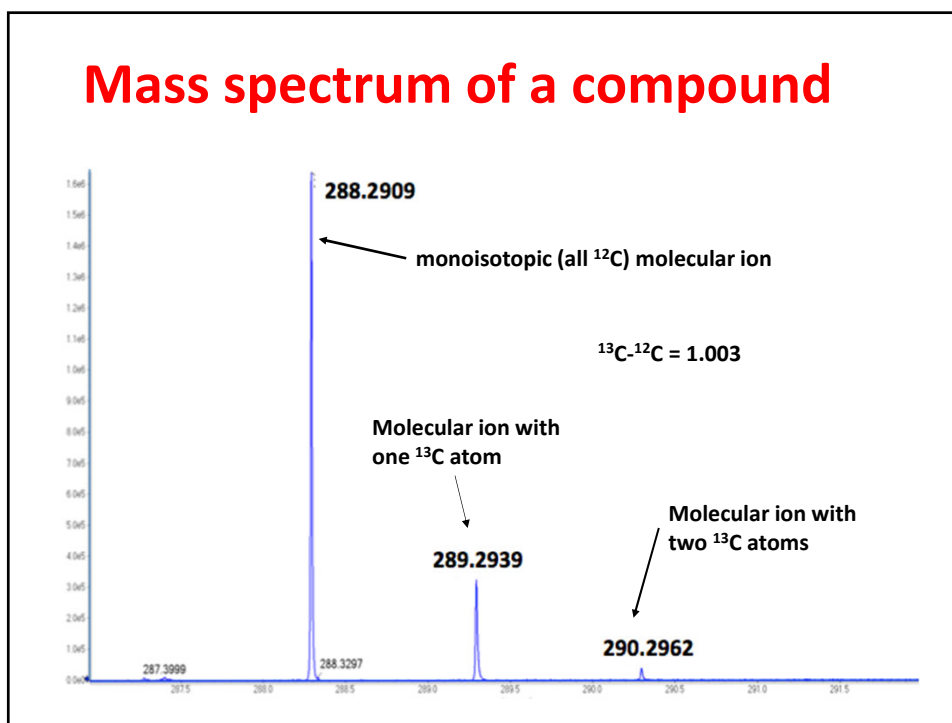

17

## Mass resolution

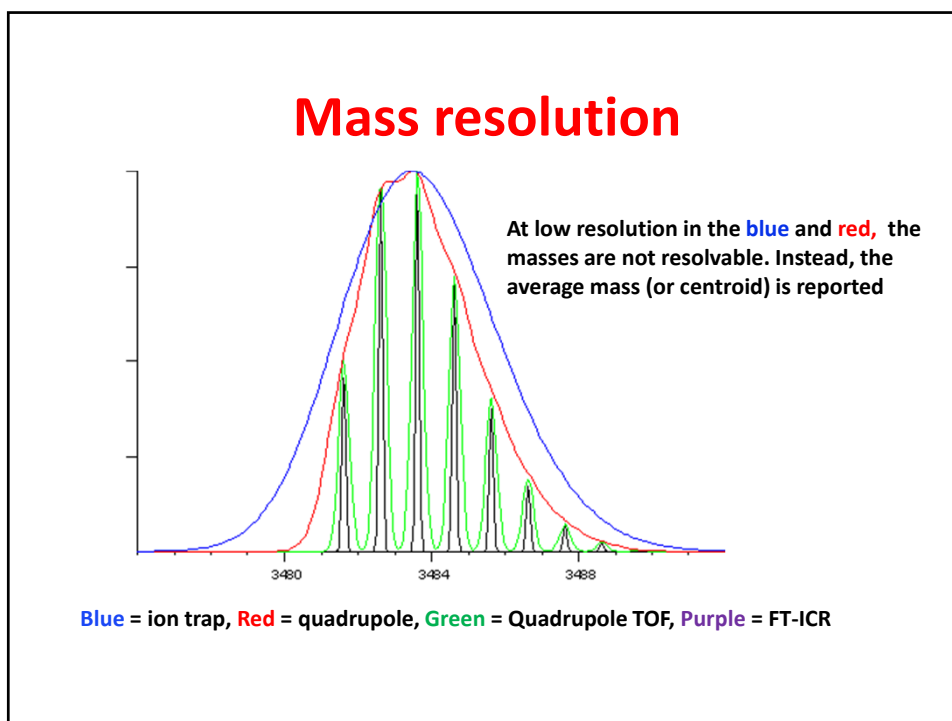


18

## Selecting the mass spectrometer

- It is necessary to use an instrument to measure:
  - The mass of the metabolites accurately
  - To provide sufficient mass resolution to distinguish the isotopes associated with each metabolite
- There are several types of MS detectors
  - Quadrupole
  - ion trap
  - time-of-flight (TOF)
  - Orbitrap
  - Fourier Transform-Ion Cyclotron Resonance (FT-ICR)

19

## Quadrupole mass filter

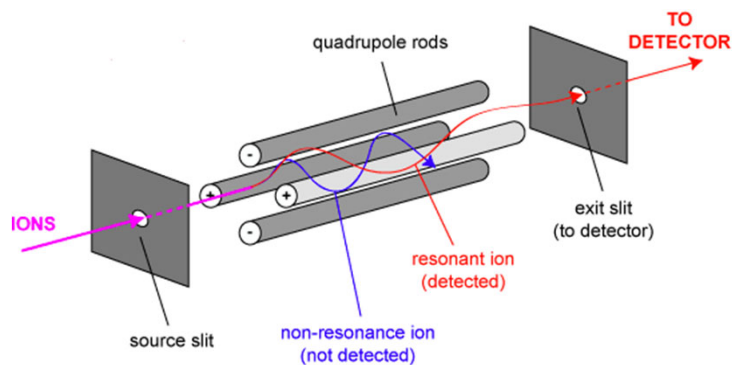


Consists of four parallel rods. Each opposing rod pair is connected together electrically, and a radio frequency (RF) voltage with a DC offset voltage is applied between one pair of rods and the other. This causes the ions to rotate in spirals as they go through the quadrupole. For a given voltage, only ions of a specific  $m/z$  can pass through. The voltage can be scanned to generate a mass spectrum or held constant to allow one ion to pass through.

20

## The mass spectrometer

- **For untargeted analysis it is important to have high mass resolution, accuracy and speed**
  - Initial data analysis is performed on the molecular ions
  - Each metabolite has a unique mass ( $m/z$ )
  - Nonetheless, a particular mass, however exact, is not necessarily a unique metabolite
- **Fourier transform-ion cyclotron resonance and Orbitrap instruments have the greatest mass accuracy**
  - However, their performance is time-dependent and is degraded significantly using short acquisition times (<100 ms)
  - They are best used for follow up experiments

21

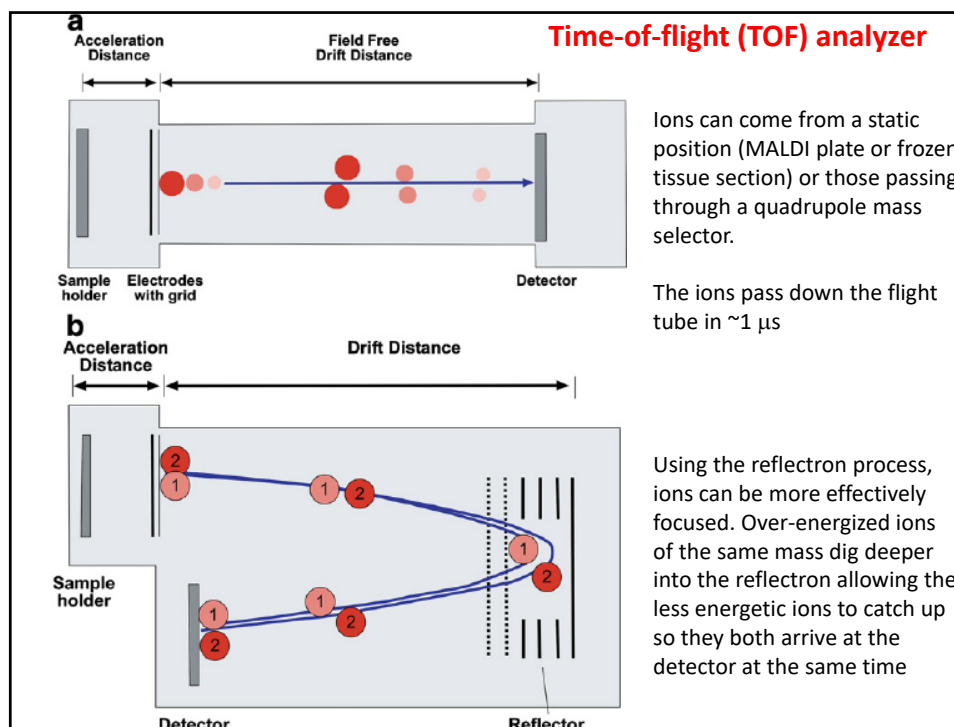

22

## TOF is the mass analyzer of choice for untargeted metabolomics

- Quadrupole-orthogonal time-of-flight (Q-tof)



Agilent 6500

Waters Synapt  
G2/HMDS

Bruker



Sciex TripleTOF 6600

Current models have 30-80,000 mass resolution and 1 ppm or better mass accuracy

23

## Links to the different Q-TOFs

- **Agilent - 6560 Ion Mobility Q-TOF LC/MS**
  - [https://www.agilent.com/cs/library/brochures/5991-3640EN\\_6560\\_Ion\\_Mobility\\_QTOF\\_LCMS\\_Brochure\\_Final\\_singlepgs.pdf](https://www.agilent.com/cs/library/brochures/5991-3640EN_6560_Ion_Mobility_QTOF_LCMS_Brochure_Final_singlepgs.pdf)
- **Bruker – TimsTof**
  - <https://www.bruker.com/products/mass-spectrometry-and-separations/lc-ms/oftof/timstof/overview.html>
- **SCIEX – 6600+ TripleTOF/SelexION**
  - <https://sciex.com/products/mass-spectrometers/qtof-systems/tripletof-systems/tripletof-6600-system>
- **Waters – Synapt G2Si**
  - [http://www.waters.com/waters/en\\_US/SYNAPT-G2-Si-High-Definition-Mass-Spectrometry/nav.htm?cid=134740622&locale=en\\_US](http://www.waters.com/waters/en_US/SYNAPT-G2-Si-High-Definition-Mass-Spectrometry/nav.htm?cid=134740622&locale=en_US)

24

## Masses of elements and their isotopes

- Mass is defined using the mass of carbon-12 being 12.0000 (exactly) – the others have non-integer mass defects
- On this scale,
  - $^1\text{H}$  is 1.007825 and  $^2\text{H}$  is 2.014102 (extra neutron)
  - $^{14}\text{N}$  is 14.003074 and  $^{15}\text{N}$  is 15.000108 (extra neutron)
  - $^{16}\text{O}$  is 15.994915,  $^{17}\text{O}$  is 16.999132 and  $^{18}\text{O}$  is 17.999161
  - $^{31}\text{P}$  is 30.973761
  - $^{32}\text{S}$  is 31.972071 and  $^{34}\text{S}$  is 33.967867 (4%)
- You can find the mass of every element and its isotopes and their natural abundances at  
<http://www.nist.gov/pml/data/comp.cfm>
- The mass of a proton is 1.0072766 and that of an electron is 0.000548597

25

## Predicted mass defects for $\text{C}_x\text{H}_n\text{O}_m$

H atoms	Oxygen atoms										
	O=0	O=1	O=2	O=3	O=4	O=5	O=6	O=7	O=8	O=9	O=10
1	0.0078	0.0027	-0.0023	-0.0074	-0.0125	-0.0176	-0.0227	-0.0278	-0.0329	-0.0379	-0.0430
2	0.0157	0.0106	0.0055	0.0004	-0.0047	-0.0098	-0.0149	-0.0199	-0.0250	-0.0301	-0.0352
3	0.0235	0.0184	0.0133	0.0082	0.0031	-0.0020	-0.0070	-0.0121	-0.0172	-0.0223	-0.0274
4	0.0313	0.0262	0.0211	0.0160	0.0110	0.0059	0.0008	-0.0043	-0.0094	-0.0145	-0.0196
5	0.0391	0.0340	0.0290	0.0239	0.0188	0.0137	0.0086	0.0035	-0.0016	-0.0066	-0.0117
6	0.0470	0.0419	0.0368	0.0317	0.0266	0.0215	0.0164	0.0114	0.0063	0.0012	-0.0039
7	0.0548	0.0497	0.0446	0.0395	0.0344	0.0294	0.0243	0.0192	0.0141	0.0090	0.0039
8	0.0626	0.0575	0.0524	0.0473	0.0423	0.0372	0.0321	0.0270	0.0219	0.0168	0.0117
9	0.0704	0.0653	0.0603	0.0552	0.0501	0.0450	0.0399	0.0348	0.0297	0.0247	0.0196
10	0.0783	0.0732	0.0681	0.0630	0.0579	0.0528	0.0477	0.0427	0.0376	0.0325	0.0274
11	0.0861	0.0810	0.0759	0.0708	0.0657	0.0607	0.0556	0.0505	0.0454	0.0403	0.0352
12	0.0939	0.0888	0.0837	0.0786	0.0736	0.0685	0.0634	0.0583	0.0532	0.0481	0.0430
13	0.1017	0.0966	0.0916	0.0865	0.0814	0.0763	0.0712	0.0661	0.0610	0.0560	0.0509
14	0.1096	0.1045	0.0994	0.0943	0.0892	0.0841	0.0790	0.0740	0.0689	0.0638	0.0587
15	0.1174	0.1123	0.1072	0.1021	0.0970	0.0920	0.0869	0.0818	0.0767	0.0716	0.0665
16	0.1252	0.1201	0.1150	0.1099	0.1049	0.0998	0.0947	0.0896	0.0845	0.0794	0.0743
17	0.1330	0.1279	0.1229	0.1178	0.1127	0.1076	0.1025	0.0974	0.0923	0.0873	0.0822
18	0.1409	0.1358	0.1307	0.1256	0.1205	0.1154	0.1103	0.1053	0.1002	0.0951	0.0900
19	0.1487	0.1436	0.1385	0.1334	0.1283	0.1233	0.1182	0.1131	0.1080	0.1029	0.0978
20	0.1565	0.1514	0.1463	0.1412	0.1362	0.1311	0.1260	0.1209	0.1158	0.1107	0.1057

For positively charged ions, add **1.007276** to the overall  $m/z$  value

For negatively charged ions, subtract **1.007276** from the overall  $m/z$  value

26

## Empirical formula

If the mass of an ion is known accurately enough, then it is possible to write down its **empirical formula**

27

## What is the mass of a metabolite?

- Hexanol

$$\begin{aligned} \text{C}_6\text{H}_{14}\text{O} &= 6 \cdot 12.0 + 14 \cdot 1.007825 + 15.994915 \\ &= 102.1044651 \end{aligned}$$

- Glucose

$$\begin{aligned} \text{C}_6\text{H}_{12}\text{O}_6 &= 6 \cdot 12.0 + 12 \cdot 1.007825 + 6 \cdot 15.994915 \\ &= 180.063388 \end{aligned}$$

28

## Masses of genistein's ions

- Genistein,  $C_{15}H_{10}O_5$

$$\text{Mass} = 15 \cdot 12.0 + 10 \cdot 1.007825 + 5 \cdot 15.994915$$

$$[M+H]^+ = M + 1.00727638 = 271.060073$$

$$[M-H]^- = M - 1.00727638 = 269.045547$$


- If glucose is joined to genistein and water ( $H_2O$ ) is eliminated, what are the values of the  $[M+H]^+$  ion and the  $[M-H]^-$  ion?
- Please send me the answer before class on Wednesday, Jan 29th.

29

## The LC

- 1D-approach

- Use of reverse-phase, normal phase and HILIC phase
- particle size – smaller is more efficient, but back pressure is a problem

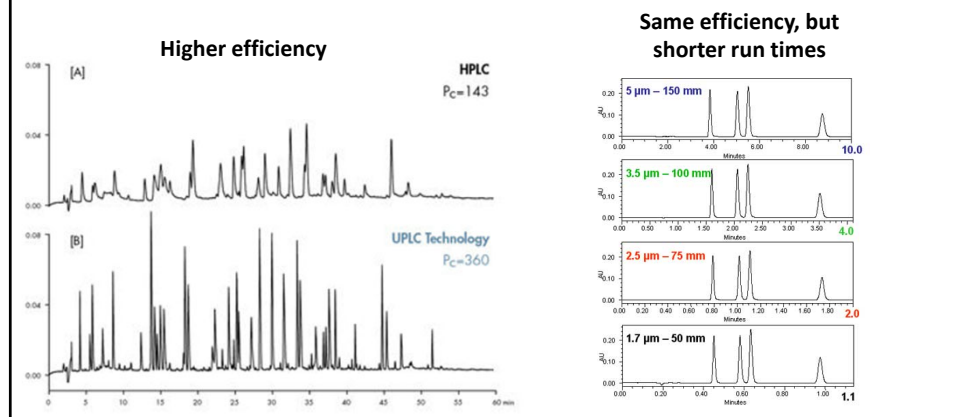

30

## LC flow rate

- MS Sensitivity is inversely related to flow rate
  - Slower flow gives more sensitivity



normal flow (0.2-0.4 ml/min)



microflow/capillary (5-50  $\mu$ l/min)




nanoflow (0.3-5  $\mu$ l/min)

31

## Improving the chromatography

- Micropillar columns

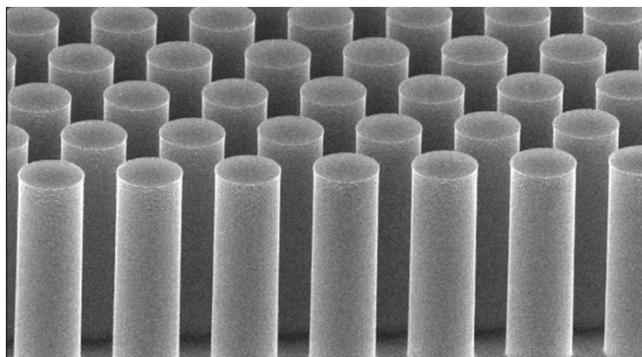


Non-turbulent fluid flow and reduced back pressure results in long-g-g columns

32



## Comparison of MP columns with other LC modes

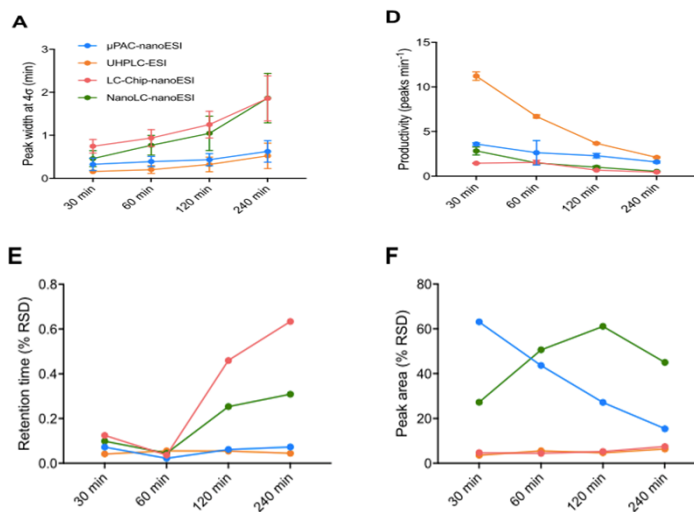

Nys G, Cobraiville G, Fillet M. Analytica Chimica Acta, 1086 (2019) 1-13


33

## Optimizing nanoLC for metabolomics


- Objective is to develop metabolomics for small animal model systems
  - *D. melangaster*
  - *C. elegans*
  - *D. rerio*
- A single zebrafish yields about 1 μl of plasma
- Need to move down to the nanoscale
- Important to maintain consistency and quantitation
  - Reproducible columns and temperature




34

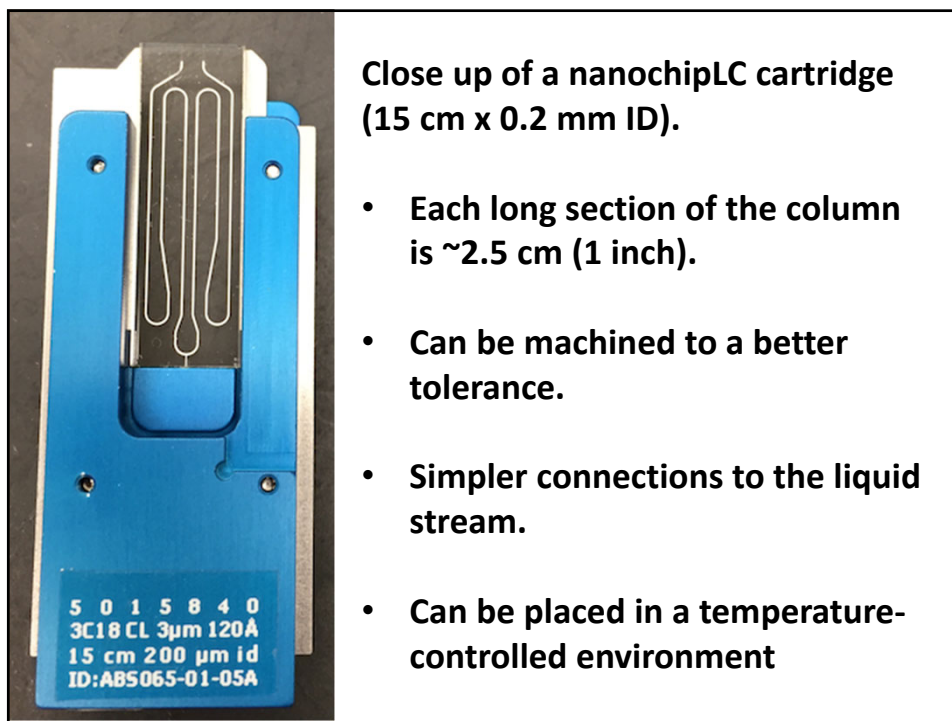


35

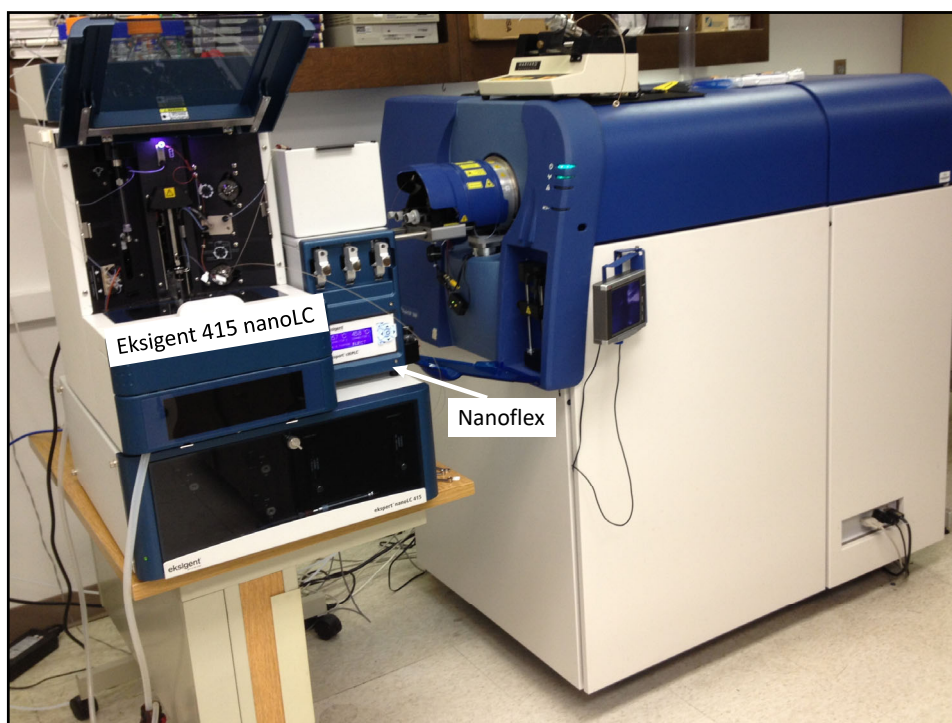


36

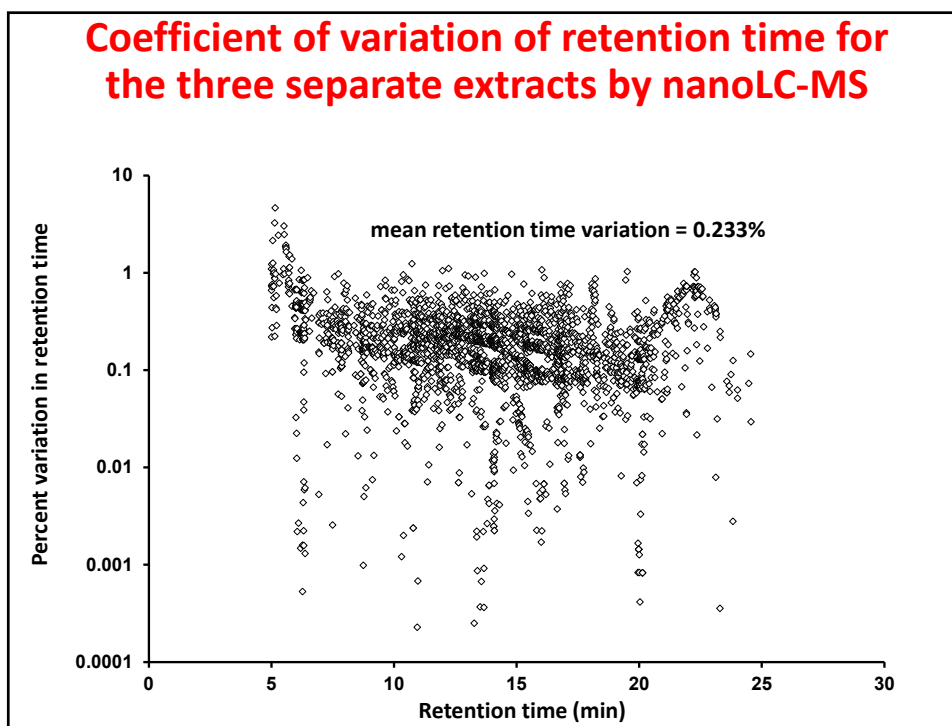


37

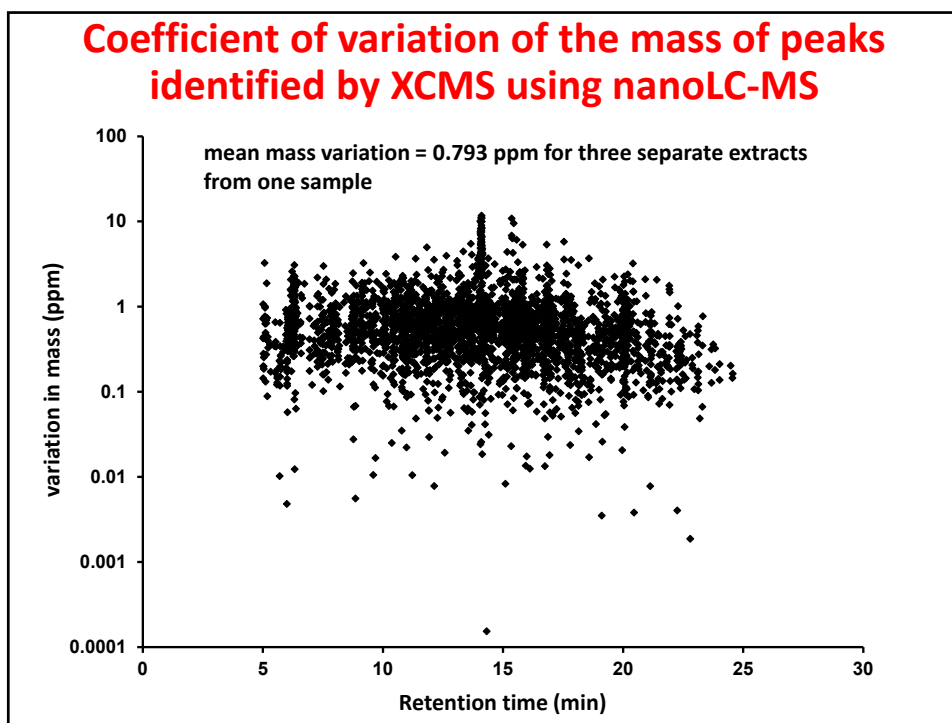

38

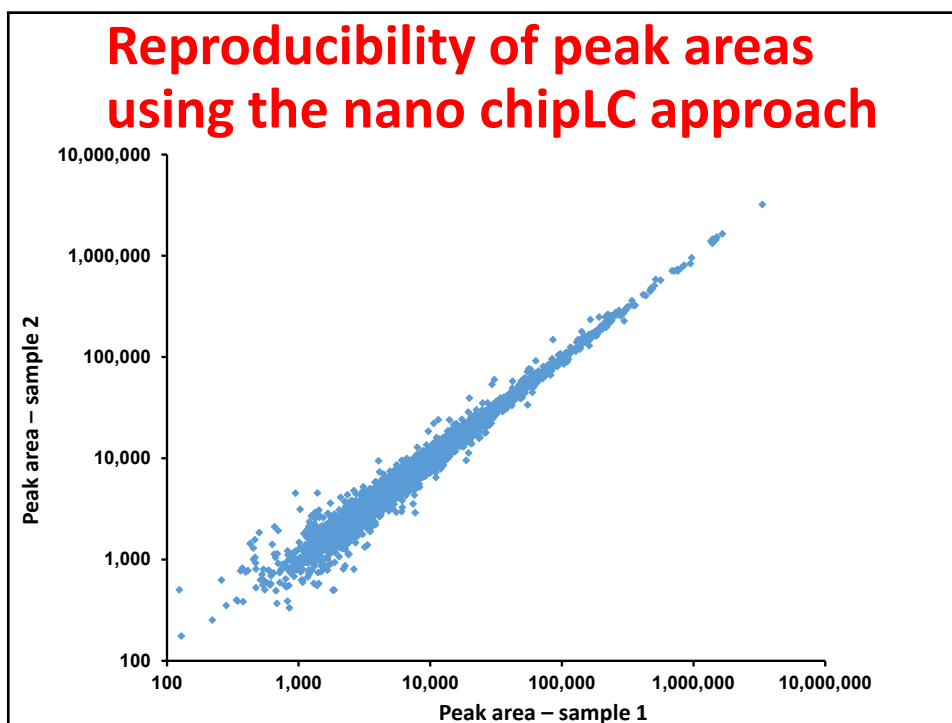


39

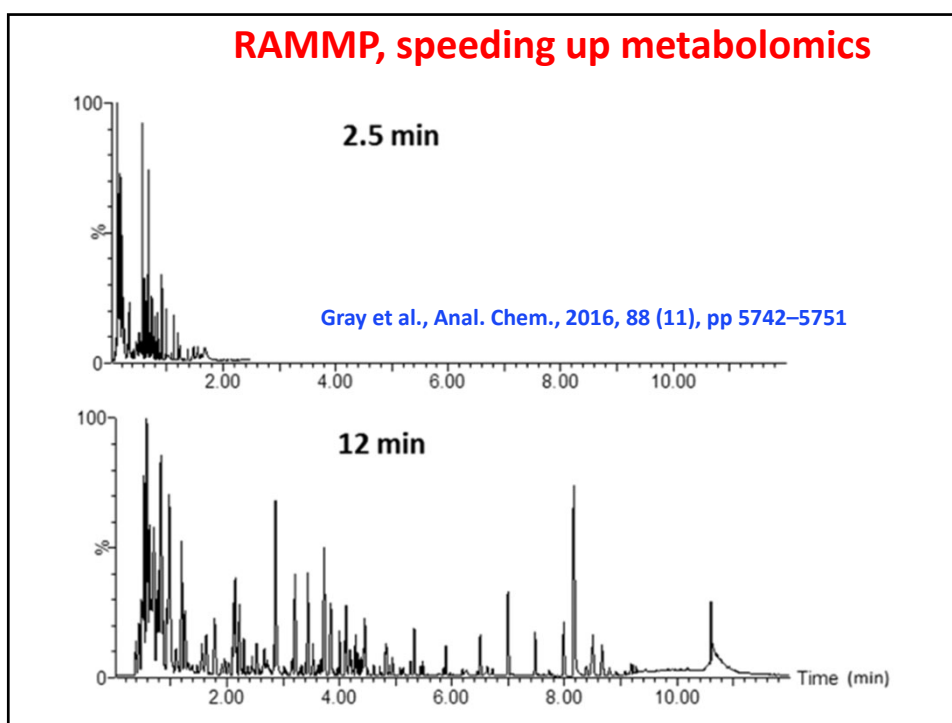

40

## RAMMP

- There was a reduction in independent features
  - 19,000 by conventional method
  - 6,000 by RAMMP

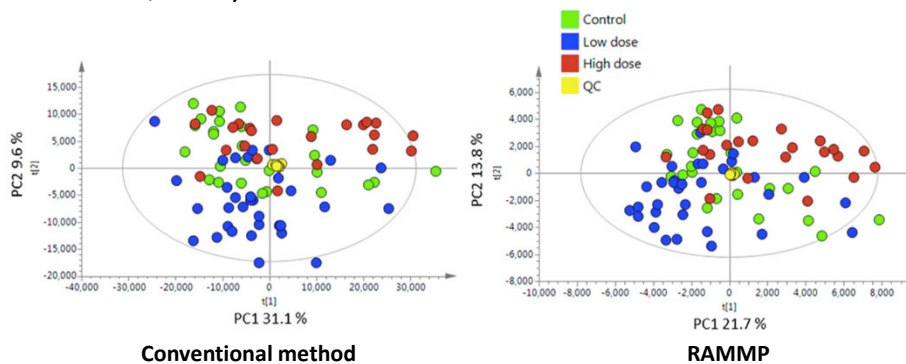


Gray et al., *Anal. Chem.*, 2016, 88 (11), pp 5742–5751

41


## Selected ion monitoring

- The summation of all the ions collected in a GC or LC analysis is called the **total ion current (TIC)** and produces a **total ion chromatogram**
- By selecting a particular mass-to-charge ratio ( $m/z$ ) value, one can see where a metabolite's molecular ion elutes from the column
  - This produces a **selected ion chromatogram (SIC or XIC)**
  - The quality of the SIC depends on the mass accuracy and resolution of the collected data


42

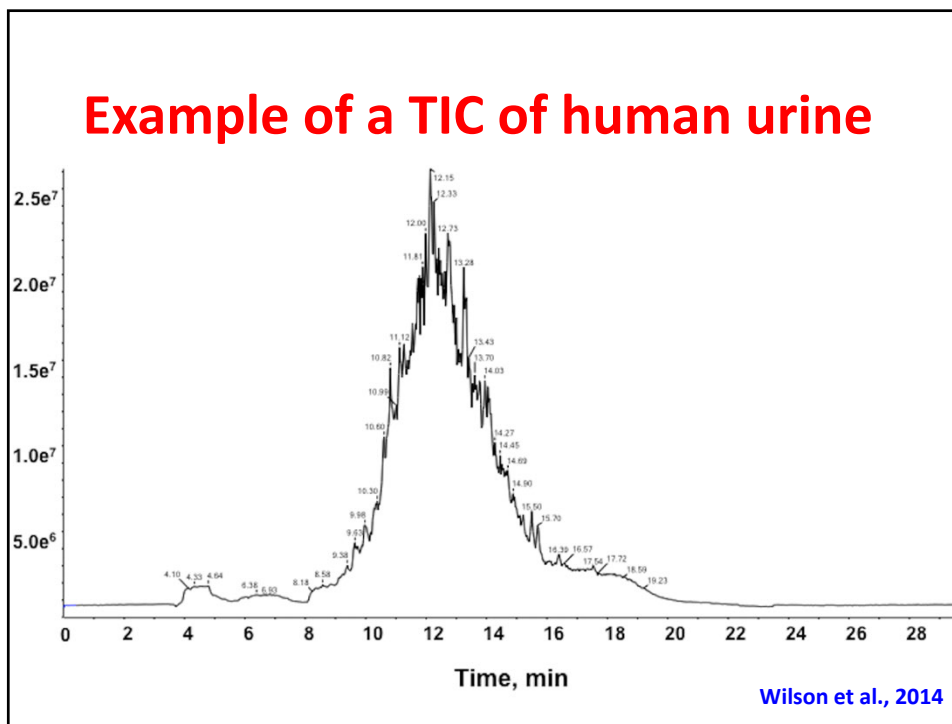

43

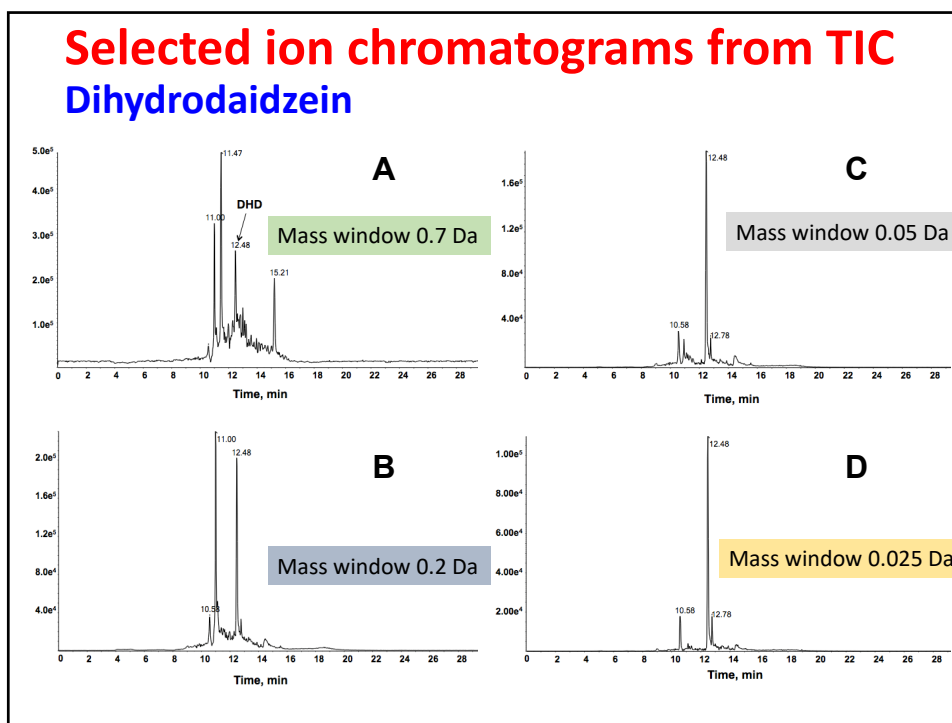

44

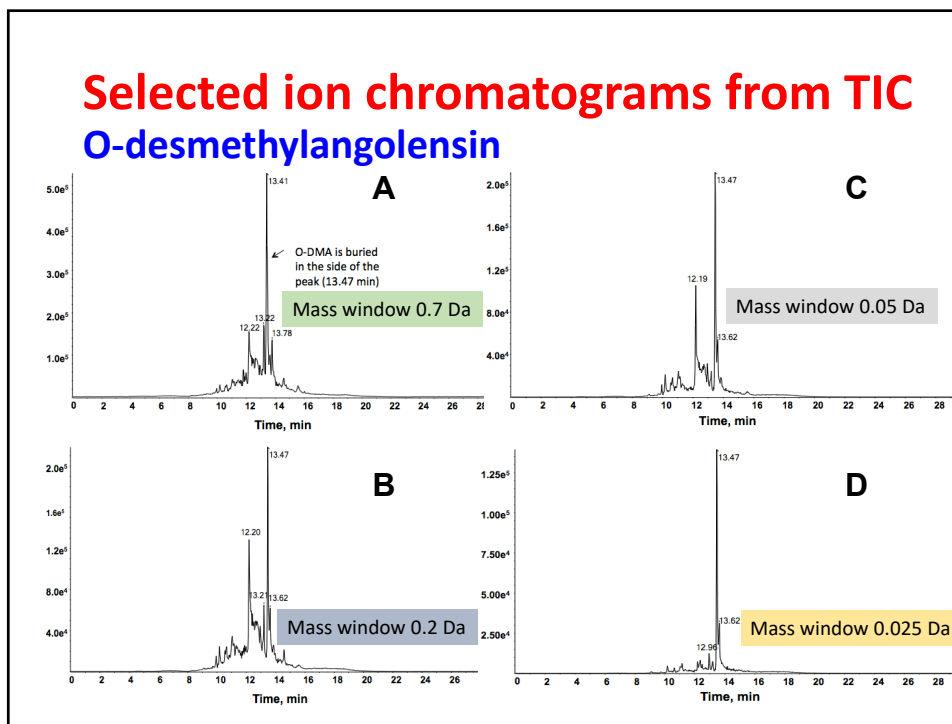


45

## MS/MS

- A second mass spectrum (MSMS) that is informative arises from isolating the molecular ion
- The molecular ion is heated, either by collision with neutral gas (quadrupole, ion traps) or by using IR radiation (FT-ICR)
  - The extra energy increases the stretching of critical bonds, leading to dissociation of the molecular precursor ion into charged product ions
  - These generate the MS/MS spectrum for a metabolite
  - Ion traps can also isolate a product ion and create MS<sup>n</sup> spectra

46

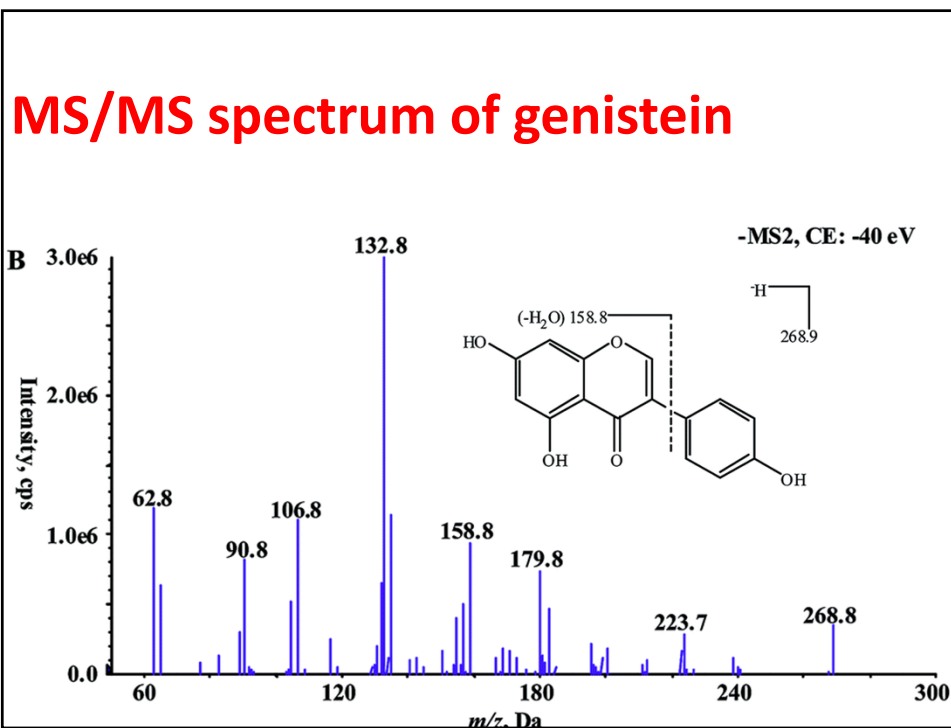

47

## Measuring a mass transition

- Instead of measuring the full MS/MS spectrum, ions from the MS/MS can be individually measured
- This is referred to as a **mass transition** from the molecular or precursor ion to a specific product ion
- It is also known as **reaction ion monitoring**

48



## Targeted vs untargeted methods


- If we know what the metabolites to be measured are (from previous untargeted analyses, or prior knowledge), then a **multiple reaction monitoring (MRM)** approach is the best way to go since allows quantitative analysis of possibly 100s of metabolites
- If there is no hypothesis, but instead you want to generate hypotheses, then the untargeted approach is better.

49

## Multiple reaction ion monitoring



Quantitative analysis of metabolites in a complex mixture carried out using a triple quadrupole instrument

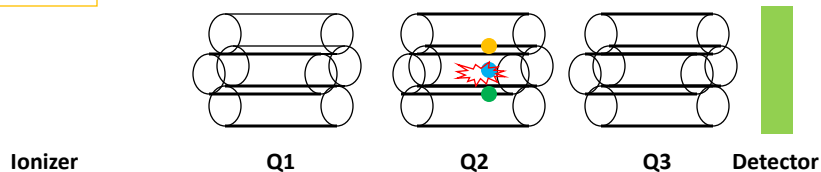

Based on precursor ion/product ion pair(s)

*Courtesy, John Cutts*


50

## How many MRM transitions?

- Acquisition can be as little as 2 msec, but acquisition time determines sensitivity
- Fast switching electronics can measure as many as 500 different transitions per second
- Since measuring the area under a peak requires 10 data points, the number of transitions measured has to be matched against the shape and width of the chromatographic peaks – to be discussed in more detail later

51


## Combined channels for Krebs cycle

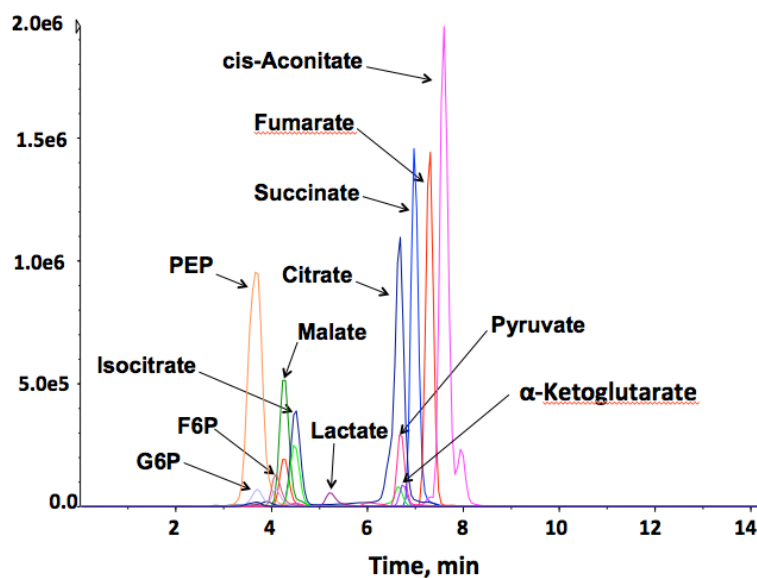

52


## Ion mobility – another parameter

53

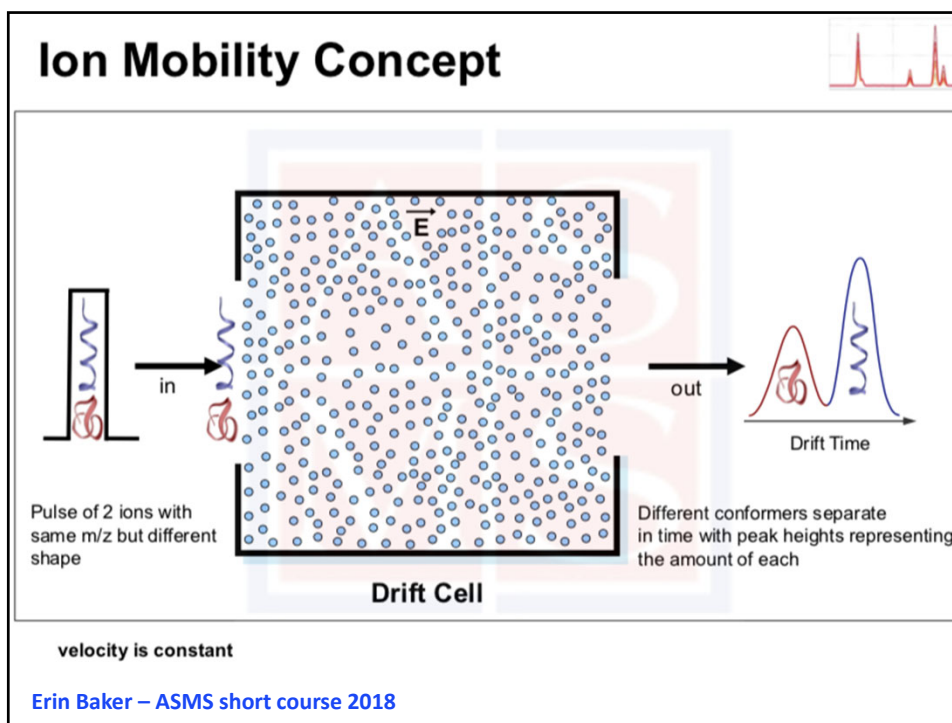

54


## Ion Mobility Concept

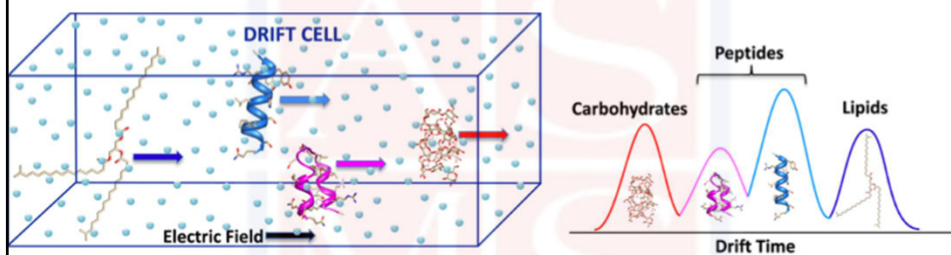


Erin Baker – ASMS short course 2018

55

## Electrodynamic time-dispersive IM-MS (TWIM-MS)

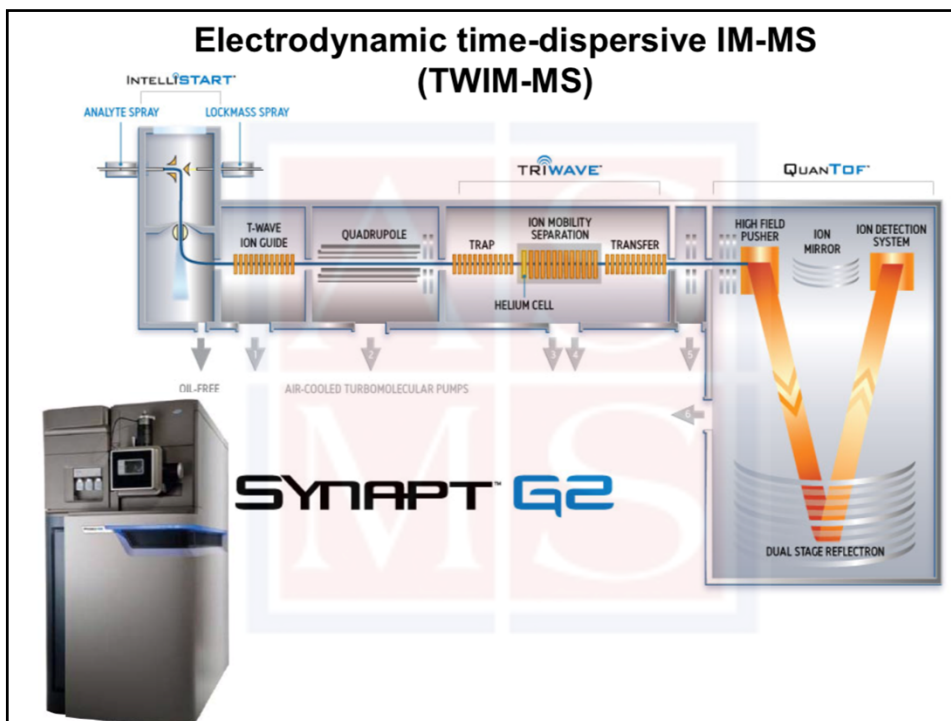

56

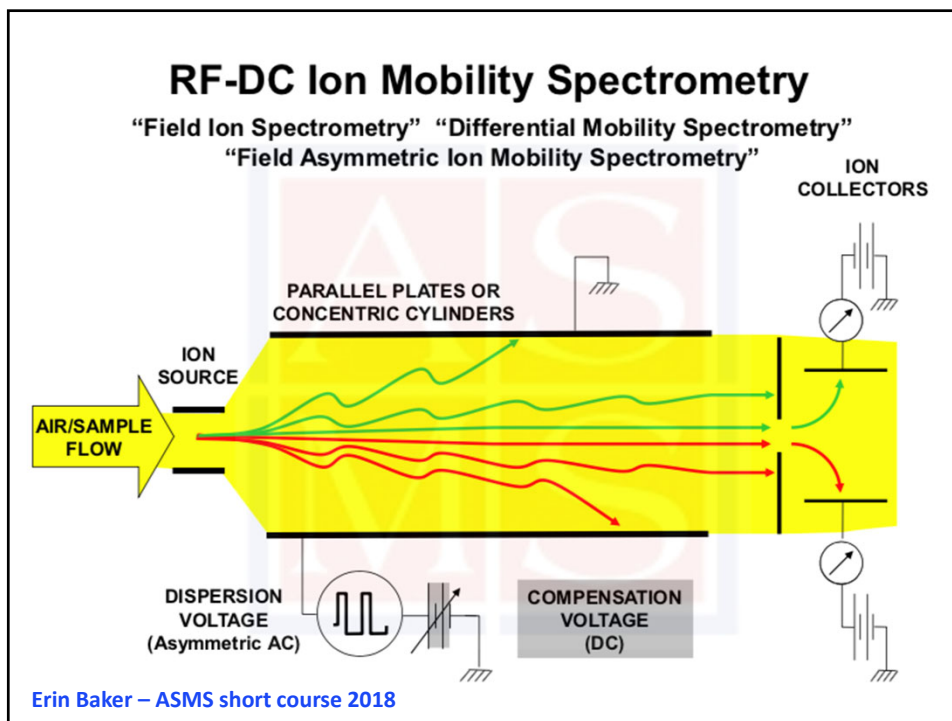


57

## Ion mobility mass spectrometry

Another method of separating classes of compounds as well as compounds with the same molecular mass


Experiment: MRM scan of 6 phospholipid standards with COV ramp

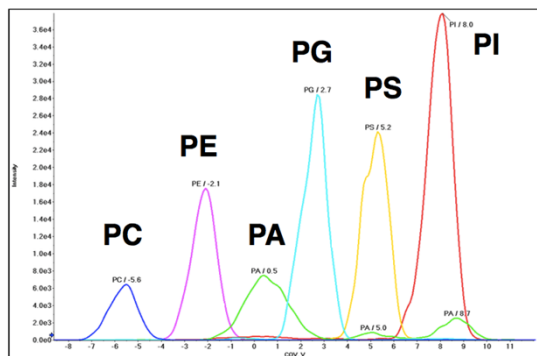


This is a gas-phase separation of these phospholipids, i.e., no chromatography.

SCIEX use a differential mobility process.

58

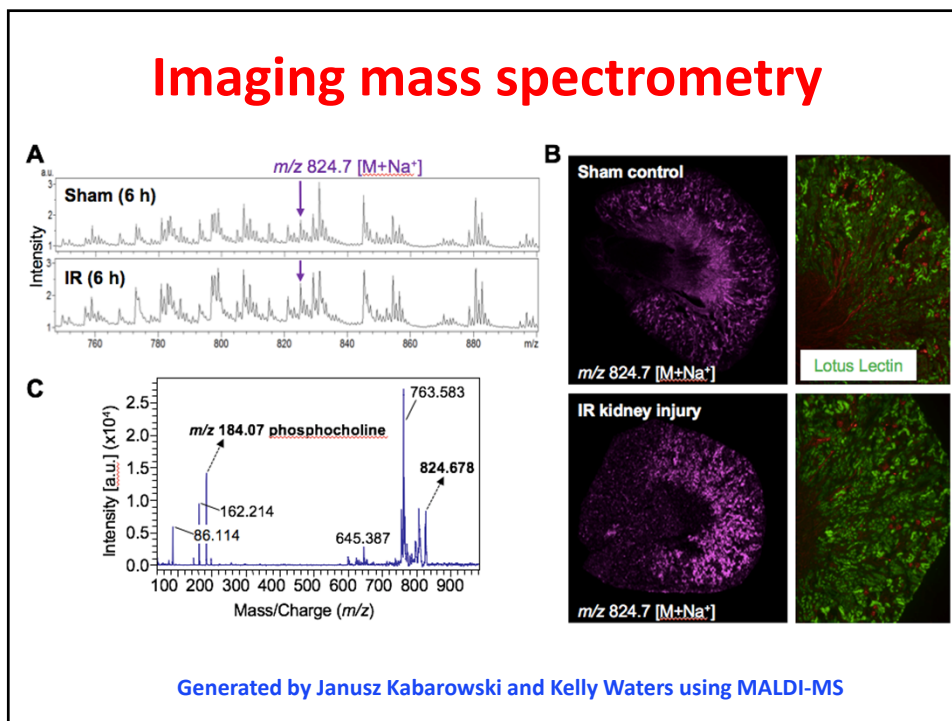


59

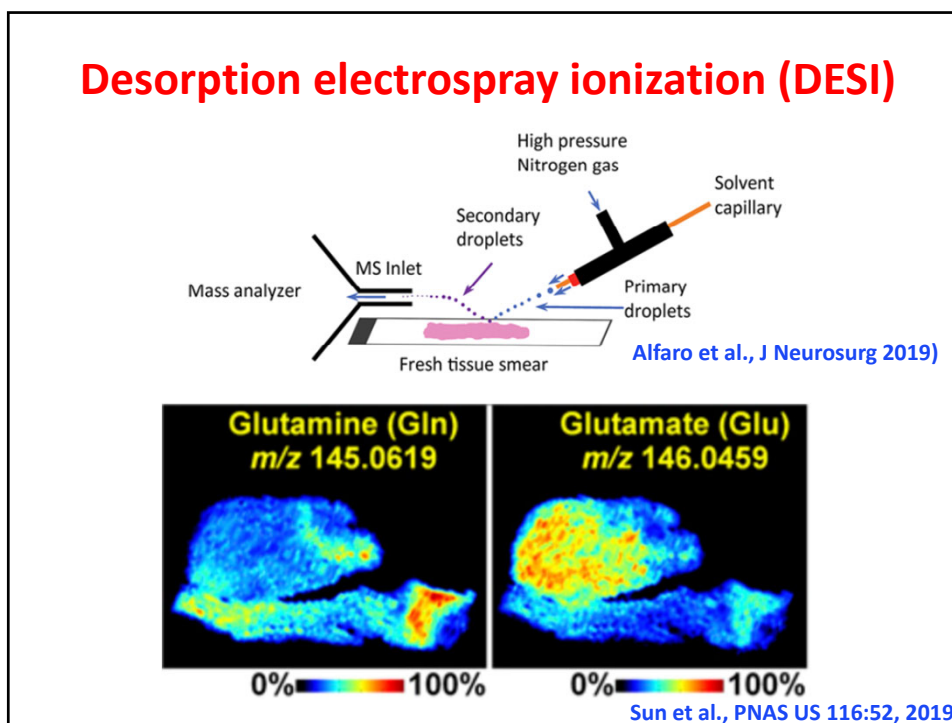

60

## Future methods in metabolomics


- Capillary electrophoresis (CE-MS)

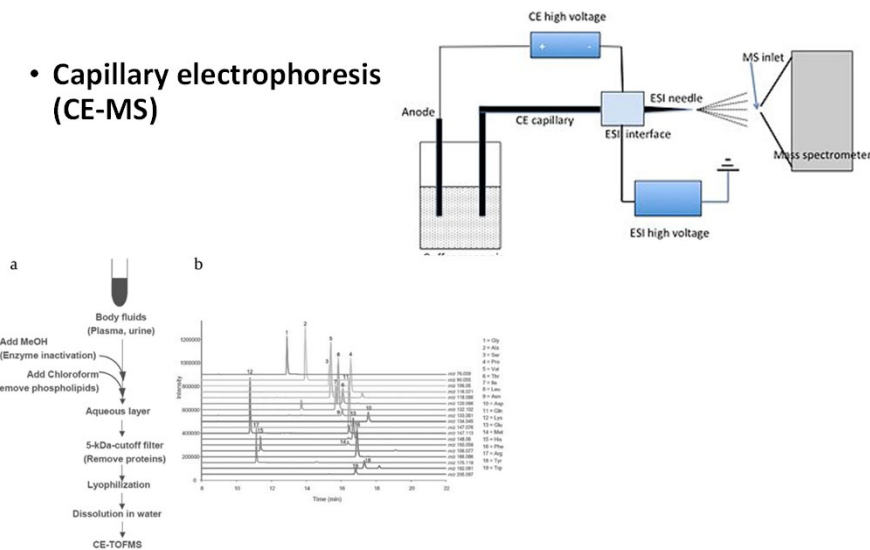

61


## Single-cell MS for Metabolomics

### In Vacuo

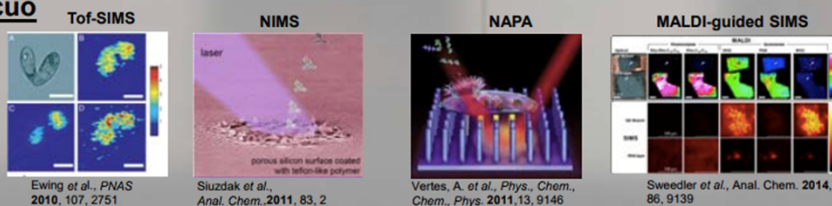


### At Ambient Conditions

- Fast analysis
- *In situ* studies

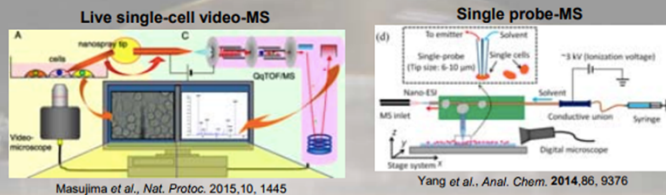

- Reduce sample complexity
  - Differentiate isobaric ions
  - Aid identifications

Courtesy of Peter Nemes



Vertes et al., Analyst, 2014, 139, 5079

- **CE-ESI-MS**
  - Minimize matrix effects
  - Aid Identifications

62

## Imaging metabolites in real time

- **In an ideal world, we want to measure metabolites without their degradation, spatially (preferably sub-cellularly) and with regard to time**
  - MS has high qualitative mass resolution and sensitivity, but it is destructive and not subcellular. Has poor time resolution
  - NMR is non-destructive and quantitative, but is not sensitive and not subcellular. Poor time resolution
- **Correlated anti-Stokes Raman Spectroscopy**
  - <https://bernstein.harvard.edu/research/cars-why.htm>
  - Is nondestructive, has high sensitivity and spatial and time resolution, but poor qualitative resolution (distinguishing metabolites)